

# Fiscal Year 2005 Solar Radiometry and Metrology Task Accomplishments

D. Myers, A. Andreas, I. Reda, P. Gotseff,  
S. Wilcox, T. Stoffel, M. Anderberg, and B. Kay  
*National Renewable Energy Laboratory*

A. Bowen  
*Baylor University*

*Presented at the 2005 DOE Solar Energy Technologies  
Program Review Meeting  
November 7–10, 2005  
Denver, Colorado*

**Conference Paper**  
**NREL/CP-560-38817**  
**November 2005**

NREL is operated by Midwest Research Institute • Battelle Contract No. DE-AC36-99-GO10337



## NOTICE

The submitted manuscript has been offered by an employee of the Midwest Research Institute (MRI), a contractor of the US Government under Contract No. DE-AC36-99GO10337. Accordingly, the US Government and MRI retain a nonexclusive royalty-free license to publish or reproduce the published form of this contribution, or allow others to do so, for US Government purposes.

This report was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or any agency thereof.

Available electronically at <http://www.osti.gov/bridge>

Available for a processing fee to U.S. Department of Energy and its contractors, in paper, from:

U.S. Department of Energy  
Office of Scientific and Technical Information  
P.O. Box 62  
Oak Ridge, TN 37831-0062  
phone: 865.576.8401  
fax: 865.576.5728  
email: <mailto:reports@adonis.osti.gov>

Available for sale to the public, in paper, from:

U.S. Department of Commerce  
National Technical Information Service  
5285 Port Royal Road  
Springfield, VA 22161  
phone: 800.553.6847  
fax: 703.605.6900  
email: [orders@ntis.fedworld.gov](mailto:orders@ntis.fedworld.gov)  
online ordering: <http://www.ntis.gov/ordering.htm>



# Fiscal Year 2005 Solar Radiometry and Metrology Task Accomplishments

D. Myers,<sup>1</sup> A. Andreas,<sup>1</sup> I. Reda,<sup>1</sup> P. Gotseff,<sup>1</sup> S. Wilcox,<sup>1</sup> T. Stoffel,<sup>1</sup> M. Anderberg,<sup>1</sup> B. Kay,<sup>1</sup> and A. Bowen<sup>2</sup>

<sup>1</sup>National Renewable Energy Laboratory, Golden, Colorado, [daryl\\_myers@nrel.gov](mailto:daryl_myers@nrel.gov)

<sup>2</sup>School of Engineering and Computer Science, Baylor University, Waco, Texas

## ABSTRACT

The National Renewable Energy Laboratory (NREL) Solar Radiometry and Metrology task provides traceable optical radiometric calibrations and measurements to photovoltaic (PV) researchers and the PV industry. Traceability of NREL solar radiometer calibrations to the World Radiometric Reference (WRR) was accomplished during Pyrheliometer Comparison at NREL in October 2004. Ten spectral and more than 200 broadband radiometers for solar measurements were calibrated this year. We measured detailed spectral distributions of the NREL and PV industry Pulsed Solar Simulators and are analyzing the influence of environmental variables on radiometer uncertainty. New systems for indoor and outdoor solar radiometer calibrations and ultraviolet (UV) spectral measurements and UV radiometer calibrations were purchased and tested. Optical metrology functions support the NREL Measurement and Characterization Task effort for ISO 17025 accreditation of NREL Solar Reference Cell Calibrations and have been integrated into the NREL quality system and audited for ISO17025 compliance.

### 1. Objectives

The project addresses technical challenges regarding analysis tools, access to data, uncertainty of analysis, standardization of assumptions, and characterization of solar resource on technologies. We provide technical expertise and input to standards and codes development to address technical issues regarding solar radiation data and measurements affecting the Fundamental Research, Advance Materials and Devices, and Technology Development components of the *Solar Program Multi-Year Technical Plan* for Flat Plate Photovoltaics, Concentrating Solar Power Systems, Solar Heating and Lighting, and New Concepts. Our objective is to provide best estimates of uncertainty and most accurate, as appropriate, optical radiation measurements and data that meet the needs of solar researchers and industry partners.

### 2. Technical Approach

Our approach is to meet solar research and industry needs in optical calibrations and measurements by providing calibrations and data of known uncertainty that is traceable to national standardizing laboratories and internationally recognized reference standards, such as the National Institute of Standards and Technology (NIST) Standard of Spectral Irradiance and the World Radiometric Reference (WRR). We participate with consensus standards organizations, in accordance with Office of Management and Budget Circular OMB A-119.<sup>1</sup> These include the American Society for Testing

and Materials (ASTM), International Standards Organization (ISO), and International Lighting Commission (CIE), which develop standards ensuring high-quality solar energy industry products. Reference standard and working instruments and systems are characterized and calibrated with documented procedures against national and international standards with as short a "traceability chain" as possible to accurately quantify and reduce uncertainties. Calibrations, measurements, and technical expertise are provided on a programmed and as-requested basis to meet the requirements for ISO 17025 accreditation.

### 3. Results and Accomplishments

Accomplishments include the following: (1) verified the stability of NREL solar radiometric reference with respect to the WRR, (2) characterized pulse solar simulator spectral distributions, (3) tested models to account for environmental influences on zero drift of pyrheliometers to measure direct solar beam, (4) tested new broadband radiometer calibration systems for outdoor and indoor calibrations, and spectral UV measurements, and (5) specified and selected new spectroradiometer system to replace obsolescent systems used in PV Measurements and Characterization task for Reference PV Cell calibrations. Successful external and internal audits resulted in the ISO 17025 accreditation for two activities in the PV Measurements and Characterization task.

#### 3.1 WRR Traceability

The project supported the NREL Pyrheliometer Comparison (NPC) Sept. 27 - Oct. 8, 2004. Twenty-three instruments were compared to NREL's *transfer standard group* (TSG) of absolute cavity radiometers that participated directly in International Pyrheliometer Comparisons (IPC) of the World Meteorological Organization (WMO). Pooled standard deviation of the TSG radiometers (with four from NREL) was 0.06%, confirming excellent stability of the NREL solar radiometric references. Figure 1 shows typical WRR transfer data for a participating cavity radiometer.

#### 3.2 Pulse Solar Simulator Characterization

The Pulse Analysis Spectroradiometer System (PASS) was upgraded with a more efficient integrating-sphere input, and was used to classify NREL and industry (Spire Corp., Shell Solar) flash simulators according to ASTM standard E-927. Figure 2 shows the ratio of new signal to old for the upgraded PASS input optics. We replaced the older barium sulfate (BaSO<sub>4</sub>)-coated integrating sphere with a spectrolon sphere.

<sup>1</sup> see <http://www.whitehouse.gov/omb/circulars/a119/a119.html>

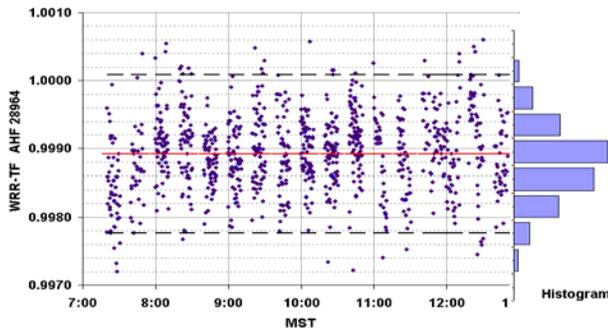


Fig. 1 Typical WRR transfer factor data for NPC 2004.

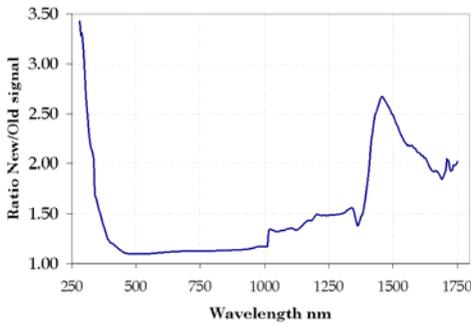


Fig. 2. Ratio of new to old throughput for improved PASS.

### 3.3 Pyrheliometer Characterization

Zero-offset signals (-5 to + 20 microvolts) are correlated with beam irradiance, rate of change of temperature, and wind speed. Five models to correct zero drift were developed from six months of 1-minute "shaded" pyrheliometer data. Models considered were independent parametric fits, multilinear regression with and without constant terms, and two component day/night, and three-component (nighttime/day low-wind/day high-wind) models. As shown in Table 1, the composite model produced the lowest mean error in correcting for zero drift.

Table 1. Mean residuals (bias error) for several model fits.

	Parametric	Day Night	Multilinear no Constant	Night Day high/low	Multilinear Constant
Count	259190	259190	259190	259190	259190
<b>Mean</b>	<b>0.00180</b>	<b>-0.0032</b>	<b>0.0115</b>	<b>0.0002</b>	<b>0.0238</b>
StDev	0.0233	0.0251	0.0251	0.02206	0.0188

### 3.4 New Radiometric Calibration Systems Performance

Three new radiometer calibration systems were implemented and tested in FY 2005: (1) new broadband outdoor radiometer calibration (BORCAL) data acquisition system (DAS) (Fig. 3a); (2) indoor pyranometer calibration system (Fig. 3b); and (3) new reference UV spectrometer. The new BORCAL DAS has 1/9th the zero offset of the previous system, and was integrated into our Radiometer Calibration and Characterization (RCC) system. Figure 4 shows that the new Kipp & Zonen indoor calibration system reproduces outdoor pyranometer calibrations with a precision of +/-2.0%. Two outlier instruments were identified for which differences of up to 7% were obtained, possibly due to spectral responsivity mismatch between the indoor lamp, outdoor sunlight, and detector paint absorption.



Fig. 3a. Afshin Andreas and new BORCAL DAS rack.



Fig 3b. Amy Bowen and Indoor Calibration System

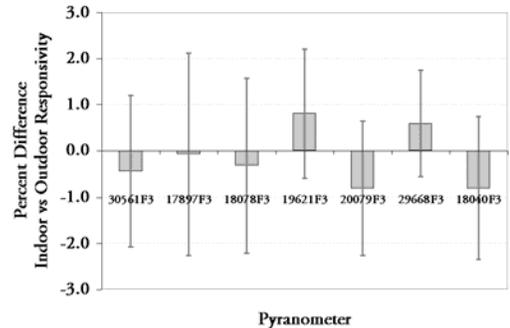


Fig. 4. Percent difference (2 sigma error bars) between BORCAL/RCC and indoor pyranometer calibration system responsivities

### 3.5. Replacement spectral measurement system

We assisted the PV measurements and characterization task with specifications and selection of a spectroradiometer system to replace obsolescent Li-COR spectrometers. As of September, 2005, a purchase order was placed for the selected system.

## 4. Conclusions

These advances assist PV researchers and industry to identify measurement artifacts, ensure accurate classification of PV products, reduce uncertainty in and improve solar radiometric data. ISO 17025 accreditation for PV reference cell calibration reinforces NREL quality data in support of the solar industry.

## ACKNOWLEDGEMENTS

This work was conducted under DOE Contract DE-AC36-99GO10337.

## MAJOR FY 2005 PUBLICATIONS

I. Reda, et al., Using a Blackbody to Calculate Net-Longwave Responsivity of Shortwave Solar Pyranometers to Correct for Thermal Offset During Outdoor Calibration Using the Component Sum Method, *Journal of Ocean Atmosphere Technology*

Myers, D.R. et al., An Update on Reducing the Uncertainty in Solar Radiometric Measurements, In *Proceedings, SOLARIS 2005*, 2nd International Conference on Solar Radiation Measurements and Models. May 25-26, Athens, Greece. Kambezidis, H. and Paissidis, G., Eds. pp 36-40. Kormos Publications, Athens, Greece.

Myers, D.R., et al. FY 2005 Midyear Progress Report Solar Radiometry and Metrology Task PVC57301 NREL/TP-56-37954 March 2005

Myers D.R., et. al. FY2005 Final Progress Report Solar Radiometry and Metrology Task PVC57301. Submitted Sep. 2005, In Press.

# REPORT DOCUMENTATION PAGE

*Form Approved*  
OMB No. 0704-0188

The public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing the burden, to Department of Defense, Executive Services and Communications Directorate (0704-0188). Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to any penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.

**PLEASE DO NOT RETURN YOUR FORM TO THE ABOVE ORGANIZATION.**

<b>1. REPORT DATE (DD-MM-YYYY)</b> November 2005		<b>2. REPORT TYPE</b> Conference Paper		<b>3. DATES COVERED (From - To)</b>	
<b>4. TITLE AND SUBTITLE</b> Fiscal Year 2005 Solar Radiometry and Metrology Task Accomplishments			<b>5a. CONTRACT NUMBER</b> DE-AC36-99-GO10337		
			<b>5b. GRANT NUMBER</b>		
			<b>5c. PROGRAM ELEMENT NUMBER</b>		
<b>6. AUTHOR(S)</b> D. Myers, A. Andreas, I. Reda, P. Gotseff, S. Wilcox, T. Stoffel, M. Anderberg, B. Kay, and A. Bowen			<b>5d. PROJECT NUMBER</b> NREL/CP-560-38817		
			<b>5e. TASK NUMBER</b> PVC5.7301		
			<b>5f. WORK UNIT NUMBER</b>		
<b>7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES)</b> National Renewable Energy Laboratory 1617 Cole Blvd. Golden, CO 80401-3393				<b>8. PERFORMING ORGANIZATION REPORT NUMBER</b> NREL/CP-560-38817	
<b>9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)</b>				<b>10. SPONSOR/MONITOR'S ACRONYM(S)</b> NREL	
				<b>11. SPONSORING/MONITORING AGENCY REPORT NUMBER</b>	
<b>12. DISTRIBUTION AVAILABILITY STATEMENT</b> National Technical Information Service U.S. Department of Commerce 5285 Port Royal Road Springfield, VA 22161					
<b>13. SUPPLEMENTARY NOTES</b>					
<b>14. ABSTRACT (Maximum 200 Words)</b> The National Renewable Energy Laboratory (NREL) Solar Radiometry and Metrology task provides traceable optical radiometric calibrations and measurements to photovoltaic (PV) researchers and the PV industry. Traceability of NREL solar radiometer calibrations to the World Radiometric Reference (WRR) was accomplished during Pyrheliometer Comparison at NREL in October 2004. Ten spectral and more than 200 broadband radiometers for solar measurements were calibrated this year. We measured detailed spectral distributions of the NREL and PV industry Pulsed Solar Simulators and are analyzing the influence of environmental variables on radiometer uncertainty. New systems for indoor and outdoor solar radiometer calibrations and ultraviolet (UV) spectral measurements and UV radiometer calibrations were purchased and tested. Optical metrology functions support the NREL Measurement and Characterization Task effort for ISO 17025 accreditation of NREL Solar Reference Cell Calibrations and have been integrated into the NREL quality system and audited for ISO17025 compliance.					
<b>15. SUBJECT TERMS</b> Photovoltaics; solar; solar radiometry; PV; NREL					
<b>16. SECURITY CLASSIFICATION OF:</b>			<b>17. LIMITATION OF ABSTRACT</b> UL	<b>18. NUMBER OF PAGES</b>	<b>19a. NAME OF RESPONSIBLE PERSON</b>
<b>a. REPORT</b> Unclassified	<b>b. ABSTRACT</b> Unclassified	<b>c. THIS PAGE</b> Unclassified			<b>19b. TELEPHONE NUMBER (Include area code)</b>