

# Impact and Detection of Pyranometer Failure on PV Performance

D.C. Jordan, B. Sekulic, S.R. Kurtz

National Renewable Energy Laboratory, Golden, CO 80401, USA

## 1 Introduction

Long-term PV Performance

- Financially:**  
Cash flow  
Uncertainty directly related to risk
- Technically:**  
Lifetime prediction  
Product improvement


Pyranometers often used to measure Plane-of-array irradiance (POA)

Pyranometers are recommended to be calibrated 1-2 years

Better understand one failure mechanism we observed in the field

Find analytical signal for early-fault detection


## 4 CM10 Pyranometer

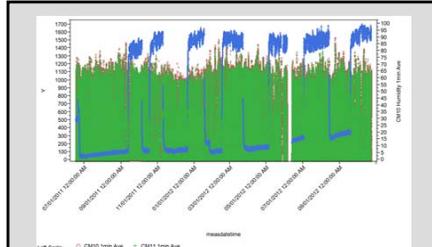

By swapping salt and desiccant, periods of high & low humidity are alternated so as not to destroy pyranometer

Use both data for PV system degradation rate determination


## 7 Detection Method

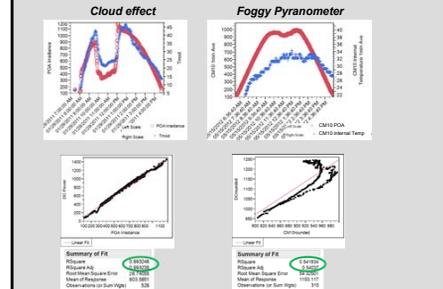

Careful tracking of R<sup>2</sup> of DC Power vs. POA

## 2 Catastrophic Failure


Field failure of pyranometer at NREL



Catastrophic field failure: Seal of SiO<sub>2</sub> cartridge failed → moisture penetrated inside

If failure not catastrophic but seal slowly disintegrates  
Could be a long time until failure is recognized!

## 5 Sunny – High Humidity

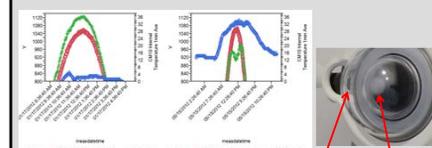


Some droplets on outer dome  
Condensation film on inner dome

On sunny days, high humidity leads to condensation that diminishes signal

Effect clearly visible on sunny days & high temperature

## 8 Detection Results

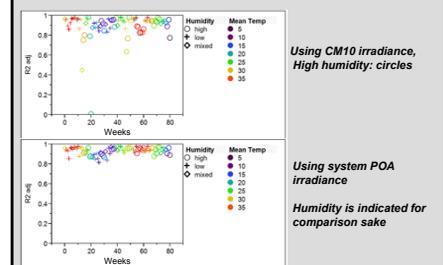

Using CM10 irradiance, High humidity: circles

Using system POA irradiance

Humidity is indicated for comparison sake

R<sup>2</sup> adj = R<sup>2</sup> adjusted for different number of data points per interval

R<sup>2</sup> adj drops significantly during pyranometer problem

## 3 Pyranometer with High Humidity

ASTM E104-85 (1996) Standard:  
Standard Practice for Maintaining Constant Relative Humidity by Means of Aqueous Solutions




Cartridge filled with desiccant SiO<sub>2</sub>  
Low humidity

Cartridge filled with saturated NaCl  
High humidity

Saturated NaCl maintains relative constant humidity in closed-spaced environment

## 6 Performance Impact

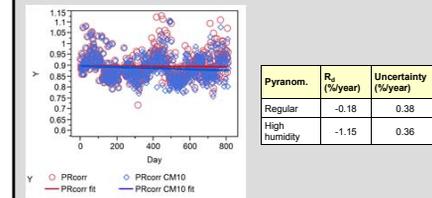

CM10 pyranometer (high humidity) drifted about 1%/year

Significant performance impact if problem is not detected

## 9 Conclusion

Accurate PV performance often depends on accurate irradiance measurements

Pyranometer with high humidity inside was used to simulate slow failure

More than 1 year of data have been collected

Pyranometer has drifted by about 1%/year

At sufficient high temperature condensation forms on inside of dome that skews data

An analytical method based on the fit of DC Power vs. POA irradiance in weekly intervals was used to detect the faulty pyranometer.